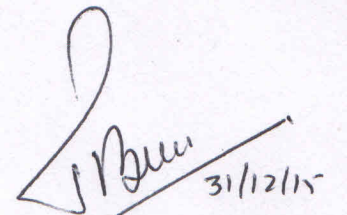


## Quotation for UV Crosslinker

Sealed quotations (technical and financial bids to be submitted separately) are invited from original equipment manufacturer or their authorised representatives for purchase of UV Crosslinker with specifications given below:

1. The unit should occupy minimum bench space with a compact footprint and a spacious interior chamber with all essential safety measures.
2. The door should have safety interlock against opening during operation and the observation window in the door should be ultraviolet blocking.
3. The unit should be compatible for fixing of nucleic acids to nylon or nitrocellulose membranes, UV mutagenesis, Gel viewing, ultraviolet curing of polymers and Ultraviolet sterilisation.
4. UV Source: 6 x 8W UV bulbs, 254, 302 or 365nm or compatible.
5. The UV exposure time should be adjusted between 0 - 999.9 min. with energy range of 0 - 99.99 J or 0 - 9.999 J.
6. The UV energy should be continuously monitored by microprocessor controlled photo feedback system to avoid variation in output from the UV sources and to ensure consistency and efficiency of operation.
7. The participating vendor should have proven after sales service record and have trained manpower.
8. Warranty: Minimum one year warranty should be included with the offer. (Cost of two years of additional warranty should be quoted as optional)
9. Prices should include transportation, customs clearance (if required) and on-site installation.
10. List of installations (preferably in the NCR region) should be provided.
11. On-site demonstration of the instrument could be asked for.

Last date for submission of quotation : **15<sup>th</sup> January 2016**

  
31/12/15

विभागाध्यक्ष / Head  
आनुवंशिकी विभाग / Department of Genetics  
दिल्ली विश्वविद्यालय दक्षिणी परिसर  
University of Delhi South Campus  
बेनिटो हुआरेज रोड / Benito Juarez Road  
नई दिल्ली-110029 / New Delhi-110021