

Quotation for UV Transilluminator

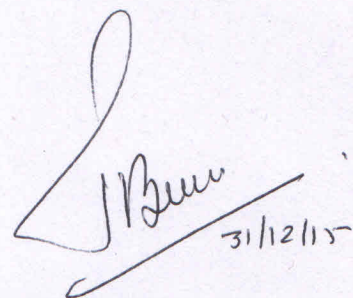
Sealed quotations (technical and financial bids to be submitted separately) are invited from original equipment manufacturer or their authorised representatives for purchase of UV Transilluminator with specifications given below:

1. The unit should have multi broad band dual wavelength UV (302 and 365nm, without changing tubes) with the ability to view a minimum of 50 nanogram of DNA
2. Imaging/viewing area should be of at least 21 x 26 cm. or better.
3. The unit should provide dual intensity (Hi/Lo) with even scan.
4. The unit should provide even illumination across the surface of transilluminator and should have a parabolic filter below the tubes for even dispersion of light.
5. The unit should have safety shield as per the standard.
6. Electric requirement: India standard.
7. The participating vendor should have proven after sales service record and have trained manpower.
8. Required accessories to operate the unit must be included in the quote.
9. Warranty: Minimum one year warranty should be included with the offer. (Cost of two years of additional warranty should be quoted as optional)
10. Prices should include transportation, customs clearance (if required) and on-site installation.
11. List of installations (preferably in the NCR region) should be provided.
12. On-site demonstration of the instrument may be required.

Optional:

Additional UV tubes: 6 UV tubes of 302 nm and 365 nm wavelength each, should be quoted as optional.

Last date for submission of quotation : **15th January 2016**


31/12/15

विभागाध्यक्ष / Head
आनुवंशिकी विभाग / Department of Genetics
दिल्ली विश्वविद्यालय दक्षिणी परिसर
University of Delhi South Campus
बेनिटो हुआरेज रोड / Benito Juarez Road
नई दिल्ली-110029 / New Delhi-110021